

Figure 1

FOLEY & LARDNER

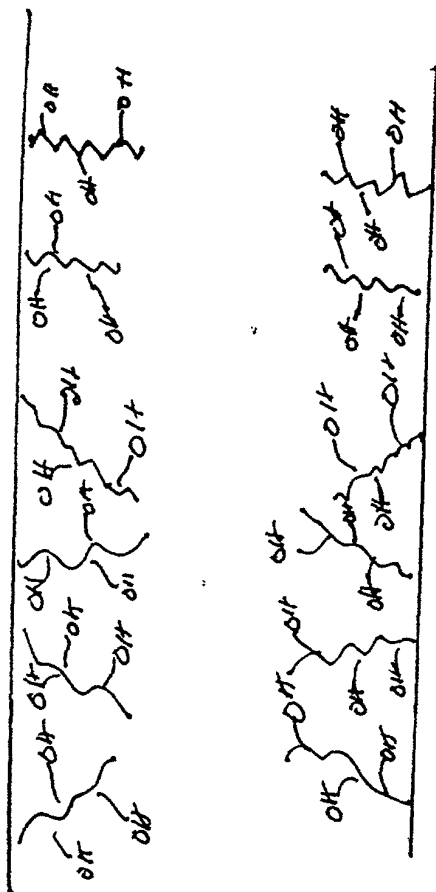


Figure 2

FOLEY & LARDNER

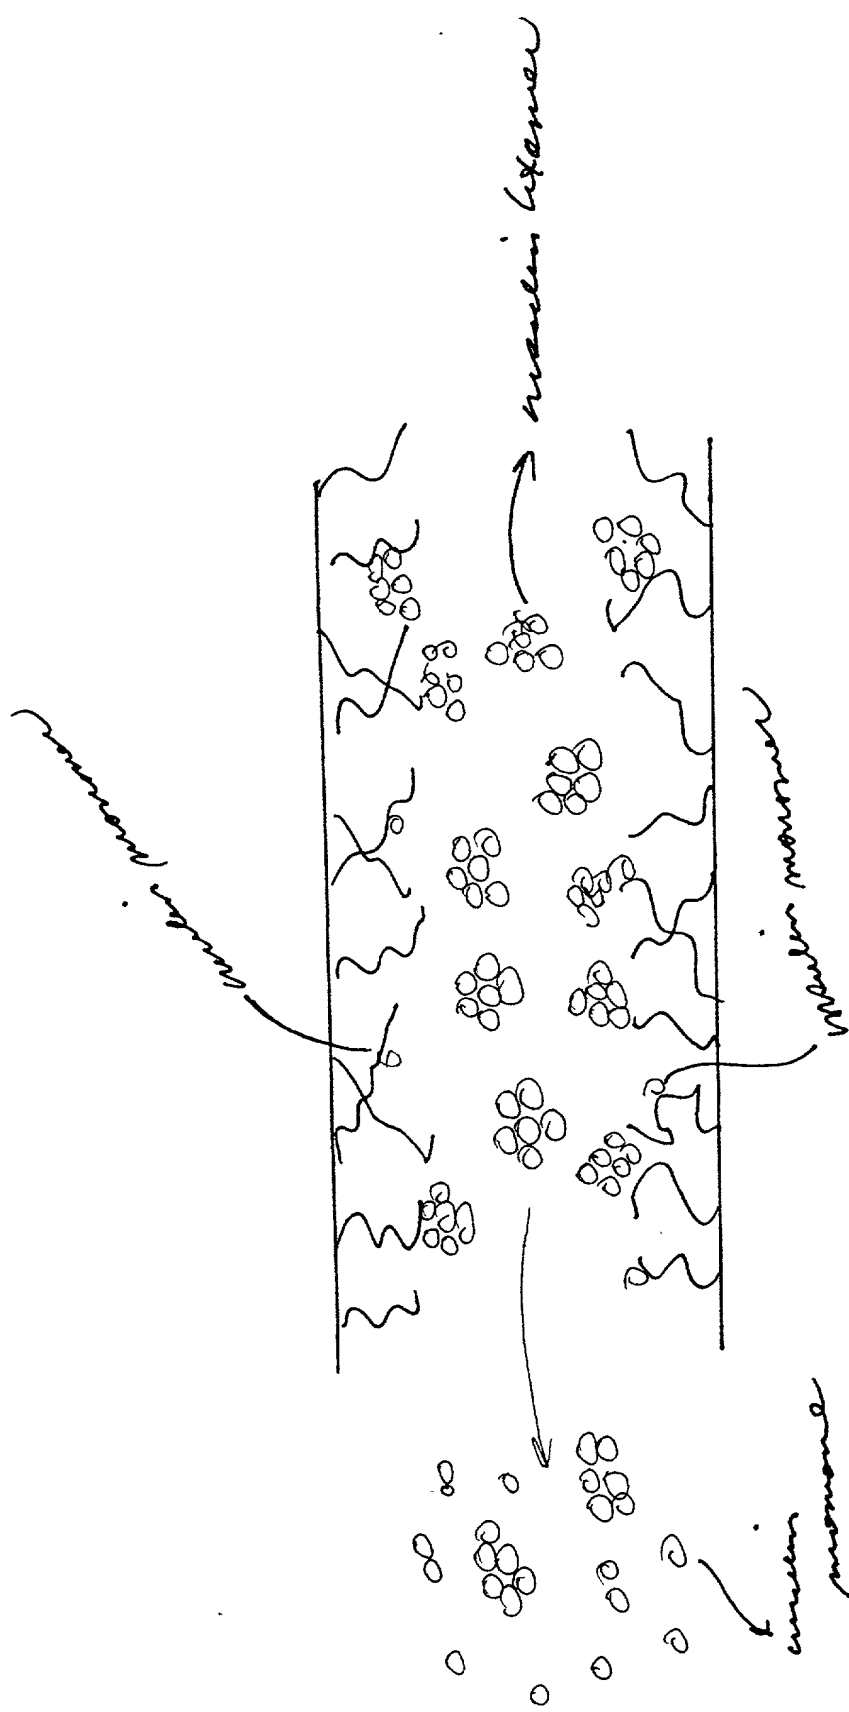


Figure 3

40035331.123804


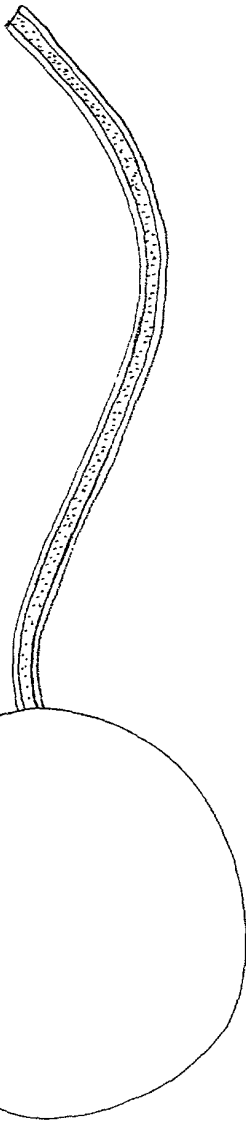



Figure 4

4055934 42301

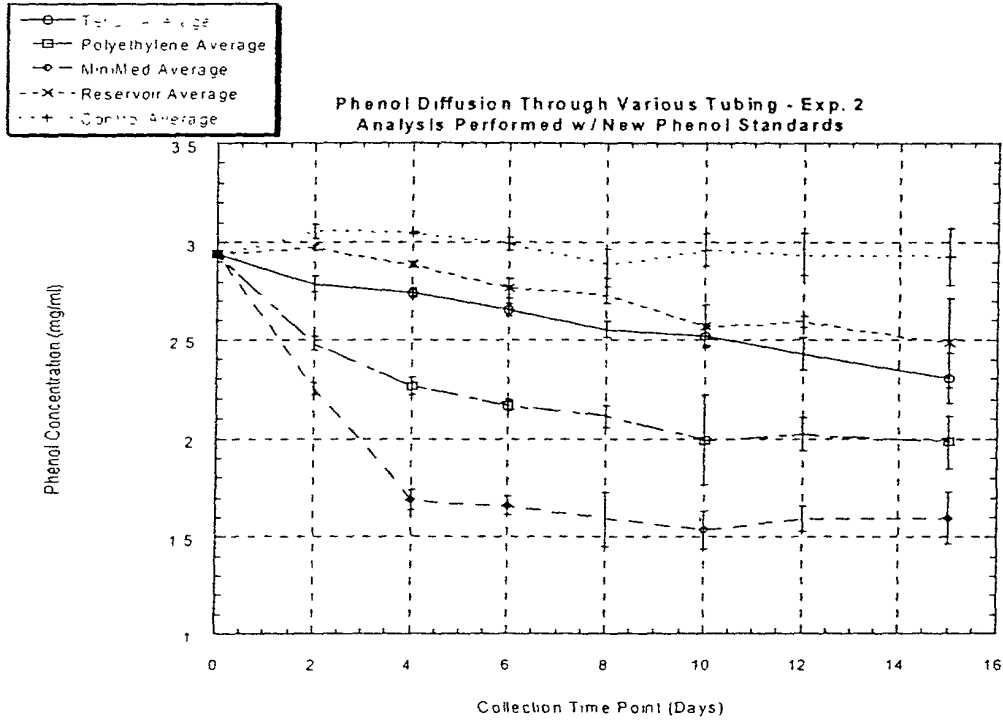

: Phenol concentration vs. time in various types of tubing as well as control and reservoir samples.

Figure 5A

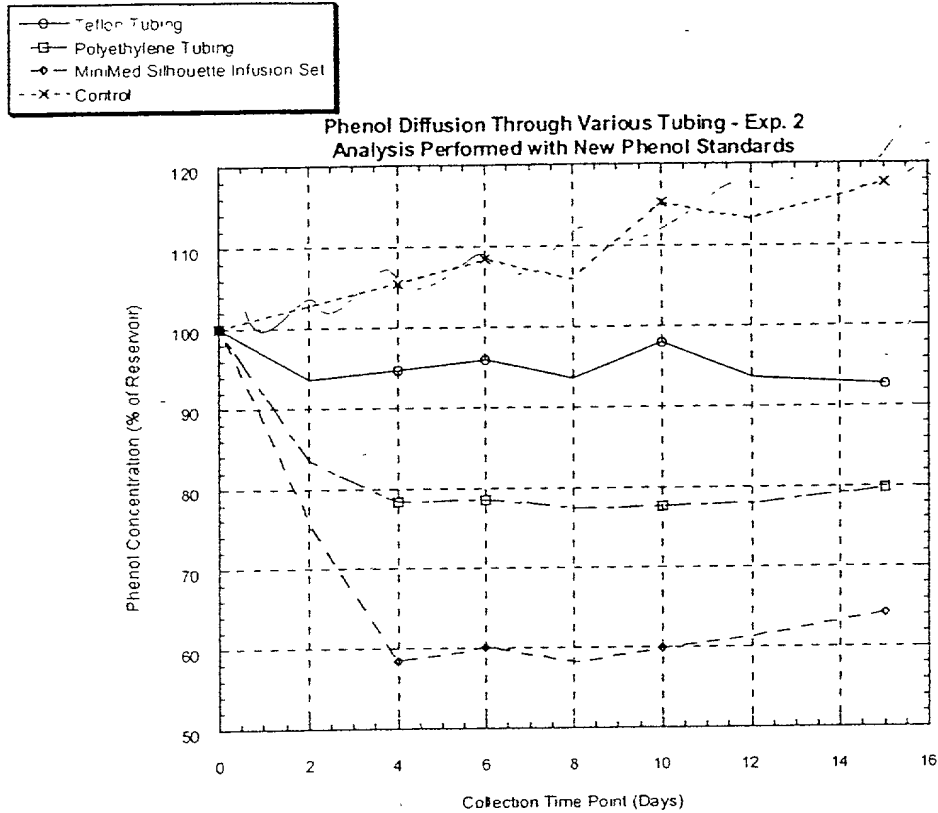

Phenol concentration as a percent of total phenol present in the reservoir vs. time in various types of tubing. A control sample is also provided for comparison.

Figure 5B

Phenol

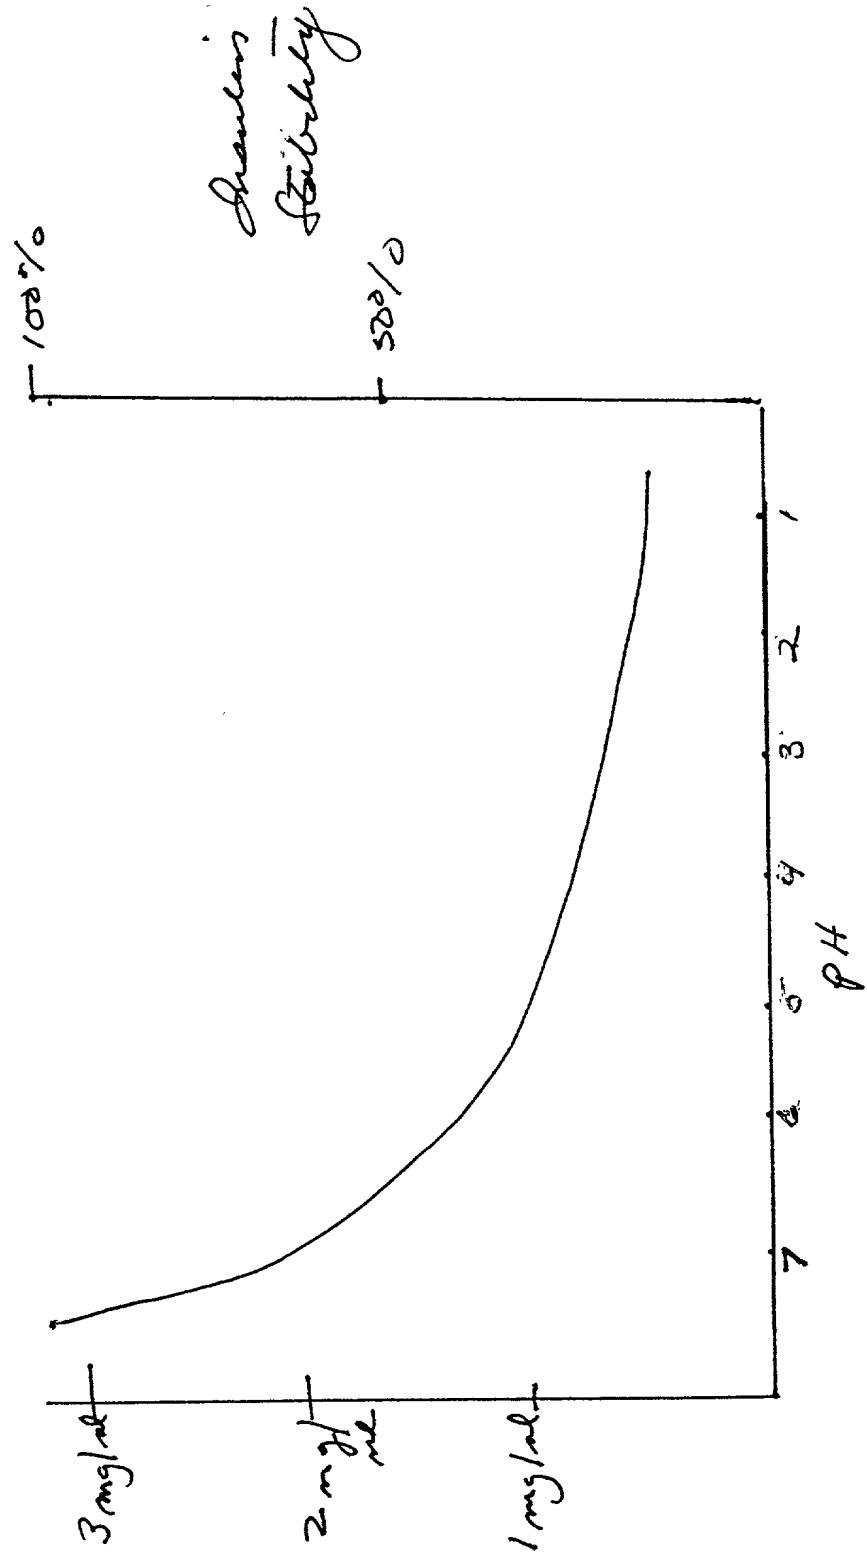


Figure 6

FOLEY & LARDNER